

HSV_{1&2} IgG

**Enzyme ImmunoAssay (ELISA) for the
quantitative/qualitative determination
of IgG antibodies to
Herpes Simplex Virus type 1 and 2
in human serum and plasma**

- for "in vitro" diagnostic use only -



DIA.PRO

**Diagnostic Bioprobes Srl
Via G. Carducci n° 27
20099 Sesto San Giovanni
(Milano) - Italy**

Phone +39 02 27007161

Fax +39 02 44386771

e-mail: info@diapro.it

REF HSVG.CE
96 Tests

HSV IgG

A. INTENDED USE

Enzyme ImmunoAssay (ELISA) for the quantitative/qualitative determination of IgG antibodies to Herpes Simplex Virus type 1 and 2 in human plasma and sera.

For "in vitro" diagnostic use only.

B. INTRODUCTION

Herpes Simplex Virus type 1 (HSV1) and type 2 (HSV2) are large complex DNA-containing viruses which have been shown to induce the synthesis of several proteins during infection, possessing an high number of crossreactive determinants and just a few of type-specific sequences.

The majority of primary and recurrent genital herpetic infections are caused by HSV2; while non genital infections, such as common cold sores, are caused primarily by HSV1.

The detection of virus specific IgG and IgM antibodies are important in the diagnosis of acute/primary virus infections or reactivations of a latent one, in the absence of evident clinical symptoms.

Asymptomatic infections may happen for HSV in apparently healthy individuals and during pregnancy. Severe herpetic infections may happen in immunocompromised and suppressed patients in which the disease may evolve toward critical pathologies.

The determination of HSV specific antibodies has then become important in the monitoring of "risk" patients and in the follow up of acute and severe infections.

C. PRINCIPLE OF THE TEST

Microplates are coated with native inactivated HSV1 and HSV2.

The solid phase is first treated with the diluted sample and IgG to HSV are captured, if present, by the antigens.

After washing out all the other components of the sample, in the 2nd incubation bound anti HSV IgG are detected by the addition of polyclonal specific anti hlgG antibodies, labelled with peroxidase (HRP).

The enzyme captured on the solid phase, acting on the substrate/chromogen mixture, generates an optical signal that is proportional to the amount of anti HSV IgG antibodies present in the sample. A Calibration Curve, calibrated against an internal Gold Standard, makes possible a quantitative determination of the IgG antibody in the patient.

D. COMPONENTS

Each kit contains sufficient reagents to perform 96 tests.

1. Microplate: MICROPLATE

n° 1. 12 strips x 8 microwells coated with native UV inactivated HSV1 and HSV2 in presence of bovine proteins.

Plates are sealed into a bag with desiccant. Allow the microplate to reach room temperature before opening; reseal unused strips in the bag with desiccant and store at 2..8°C.

2. Calibration Curve: CAL N° ...

Ready to use and color coded standard curve derived from human plasma positive for HSV IgG ranging:

4ml CAL1 = 0 arbU/ml
4ml CAL2 = 5 arbU/ml
2ml CAL3 = 10 arbU/ml
2ml CAL4 = 20 arbU/ml
2ml CAL5 = 50 arbU/ml
4ml CAL6 = 100 arbU/ml.

Standards are calibrated in arbitrary units against an internal Gold Standard (or IGS).

It contains human serum proteins, 2% casein, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.1% Tween 20, 0.09% Na-azide and 0.045% ProClin 300 as preservatives. Standards are blue colored.

3. Control Serum: CONTROL ...ml

1 vial. Lyophilized. It contains fetal bovine serum proteins, human IgG antibodies to HSV at about 20 arbU/ml ± 20%, 0.2 mg/ml gentamicine sulphate and 0.045% ProClin 300 as preservatives.

Note: The volume necessary to dissolve the content of the vial may vary from lot to lot. Please use the right volume reported on the label.

4. Wash buffer concentrate: WASHBUF 20X

1x60ml/bottle20x concentrated solution. Once diluted, the wash solution contains 10 mM phosphate buffer pH 7.0+/-0.2, 0.05% Tween 20 and 0.045% ProClin 300.

5. Enzyme conjugate : CONJ

2x8ml/vial. Ready to use and red colour coded. It contains Horseradish peroxidase conjugated polyclonal antibodies to human IgG, 5% BSA, 10 mM Tris buffer pH 6.8+/-0.1, 0.045% ProClin 300, 0.02% gentamicine sulphate as preservatives and 0.01% red alimentary dye.

6. Chromogen/Substrate: SUBS TMB

1x16ml/vial. It contains 50 mM citrate-phosphate buffer pH 3.5-3.8, 4% dimethylsulphoxide, 0.03% tetra-methyl-benzidine (or TMB) and 0.02% hydrogen peroxide (or H₂O₂) and 4% dimethylsulphoxide.

Note: To be stored protected from light as sensitive to strong illumination.

7. Sulphuric Acid: H₂SO₄ 0.3 M

1x15ml/vial. It contains 0.3 M H₂SO₄ solution.

Attention: Irritant (H315, H319; P280, P302+P352, 332+P313, P305+ P351+P338, P337+P313, P362+P363)

8. Specimen Diluent: DILSPE

2x60ml/vial. It contains 2% casein, 10 mM Na-citrate buffer pH 6.0 +/-0.1, 0.1% Tween 20, 0.09% Na-azide, 0.045% ProClin 300 as preservatives. The reagent is blue colour coded.

9. Plate sealing foils n°2

10. Package insert n°1

E. MATERIALS REQUIRED BUT NOT PROVIDED

1. Calibrated Micropipettes (1000 ul, 100 ul and 10 ul) and disposable plastic tips.
2. EIA grade water (double distilled or deionised, charcoal treated to remove oxidizing chemicals used as disinfectants).
3. Timer with 60 minute range or higher.
4. Absorbent paper tissues.
5. Calibrated ELISA microplate thermostatic incubator (dry or wet), set at +37°C (+/-0.5°C tolerance)..
6. Calibrated ELISA microwell reader with 450nm (reading) and with 620-630nm (blinking) filters.
7. Calibrated ELISA microplate washer.
8. Vortex or similar mixing tools.

F. WARNINGS AND PRECAUTIONS

1. The kit has to be used by skilled and properly trained technical personnel only, under the supervision of a medical doctor responsible of the laboratory.
2. All the personnel involved in performing the assay have to wear protective laboratory clothes, talc-free gloves and glasses.

The use of any sharp (needles) or cutting (blades) devices should be avoided. All the personnel involved should be trained in biosafety procedures, as recommended by the Center for Disease Control, Atlanta, U.S. and reported in the National Institute of Health's publication: "Biosafety in Microbiological and Biomedical Laboratories", ed. 1984.

3. All the personnel involved in sample handling should be vaccinated for HBV and HAV, for which vaccines are available, safe and effective.
4. The laboratory environment should be controlled so as to avoid contaminants such as dust or air-borne microbial agents, when opening kit vials and microplates and when performing the test. Protect the Chromogen (TMB) from strong light and avoid vibration of the bench surface where the test is undertaken.
5. Upon receipt, store the kit at 2..8°C into a temperature controlled refrigerator or cold room.
6. Do not interchange components between different lots of the kits. It is recommended that components between two kits of the same lot should not be interchanged.
7. Check that the reagents are clear and do not contain visible heavy particles or aggregates. If not, advise the laboratory supervisor to initiate the necessary procedures for kit replacement.
8. Avoid cross-contamination between serum/plasma samples by using disposable tips and changing them after each sample. Do not reuse disposable tips.
9. Avoid cross-contamination between kit reagents by using disposable tips and changing them between the use of each one. Do not reuse disposable tips.
10. Do not use the kit after the expiration date stated on the external container and internal (vials) labels. A study conducted on an opened kit did not pointed out any relevant loss of activity up to six 6 uses of the device and up to 3 months.
11. Treat all specimens as potentially infective. All human serum specimens should be handled at Biosafety Level 2, as recommended by the Center for Disease Control, Atlanta, U.S. in compliance with what reported in the Institutes of Health's publication: "Biosafety in Microbiological and Biomedical Laboratories", ed. 1984.
12. The use of disposable plastic-ware is recommended in the preparation of the liquid components or in transferring components into automated workstations, in order to avoid cross contamination.
13. Waste produced during the use of the kit has to be discarded in compliance with national directives and laws concerning laboratory waste of chemical and biological substances. In particular, liquid waste generated from the washing procedure, from residuals of controls and from samples has to be treated as potentially infective material and inactivated before waste. Suggested procedures of inactivation are treatment with a 10% final concentration of household bleach for 16-18 hrs or heat inactivation by autoclave at 121°C for 20 min..
14. Accidental spills from samples and operations have to be adsorbed with paper tissues soaked with household bleach and then with water. Tissues should then be discarded in proper containers designated for laboratory/hospital waste.
15. The Sulphuric Acid is an irritant. In case of spills, wash the surface with plenty of water
16. Other waste materials generated from the use of the kit (example: tips used for samples and controls, used microplates) should be handled as potentially infective and disposed according to national directives and laws concerning laboratory wastes.

G. SPECIMEN: PREPARATION AND WARNINGS

1. Blood is drawn aseptically by venepuncture and plasma or serum is prepared using standard techniques of preparation of samples for clinical laboratory analysis. No influence has been observed in the preparation of the sample with citrate, EDTA and heparin.

2. Samples have to be clearly identified with codes or names in order to avoid misinterpretation of results. Bar code labeling and electronic reading is strongly recommended.

3. Haemolysed ("red") and visibly hyperlipemic ("milky") samples have to be discarded as they could generate false results. Samples containing residues of fibrin or heavy particles or microbial filaments and bodies should be discarded as they could give rise to false results.

4. Sera and plasma can be stored at +2°...+8°C in primary collection tubes for up to five days after collection. Do not freeze primary tubes of collection. For longer storage periods, sera and plasma samples, carefully removed from the primary collection tube, can be stored frozen at -20°C for at least 12 months. Any frozen samples should not be frozen/thawed more than once as this may generate particles that could affect the test result.

5. If particles are present, centrifuge at 2.000 rpm for 20 min or filter using 0.2-0.8µ filters to clean up the sample for testing.

H. PREPARATION OF COMPONENTS AND WARNINGS

A study conducted on an opened kit has not pointed out any relevant loss of activity up to 6 re-uses of the device and up to 3 months.

Microplate:

Allow the microplate to reach room temperature (about 1 hr) before opening the container. Check that the desiccant has not turned dark green, indicating a defect in manufacturing. In this case, call Dia.Pro's customer service.

Unused strips have to be placed back into the aluminum pouch, with the desiccant supplied, firmly zipped and stored at +2..8°C.

After first opening, remaining strips are stable until the humidity indicator inside the desiccant bag turns from yellow to green.

Calibration Curve

Ready to use component. Mix carefully on vortex before use.

Control Serum

Add the volume of ELISA grade water, reported on the label, to the lyophilised powder; let fully dissolve and then gently mix on vortex.

Note: *The control after dissolution is not stable. Store frozen in aliquots at -20°C.*

Wash buffer concentrate:

The whole content of the concentrated solution has to be diluted 20x with bidistilled water and mixed gently end-over-end before use. During preparation avoid foaming as the presence of bubbles could impact on the efficiency of the washing cycles.

Note: *Once diluted, the wash solution is stable for 1 week at +2..8° C.*

Enzyme conjugate:

Ready to use. Mix well on vortex before use.

Be careful not to contaminate the liquid with oxidizing chemicals, air-driven dust or microbes.

If this component has to be transferred use only plastic, possibly sterile disposable containers.

Chromogen/Substrate:

Ready to use. Mix well on vortex before use.

Be careful not to contaminate the liquid with oxidizing chemicals, air-driven dust or microbes.

Do not expose to strong illumination, oxidizing agents and metallic surfaces.

If this component has to be transferred use only plastic, possible sterile disposable container

Sample Diluent

Ready to use component. Mix carefully on vortex before use.

Sulphuric Acid:

Ready to use. Mix well on vortex before use.

Attention: Irritant (H315, H319; P280, P302+P352, 332+P313, P305+ P351+P338, P337+P313, P362+P363).

Legenda:

Warning H statements:

H315 – Causes skin irritation.

H319 – Causes serious eye irritation.

Precautionary P statements:

P280 – Wear protective gloves/protective clothing/eye protection/face protection.

P302 + P352 – IF ON SKIN: Wash with plenty of soap and water.

P332 + P313 – If skin irritation occurs: Get medical advice/attention.

P305 + P351 + P338 – IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing.

P337 + P313 – If eye irritation persists: Get medical advice/attention.

P362 + P363 - Take off contaminated clothing and wash it before reuse.

I. INSTRUMENTS AND TOOLS USED IN COMBINATION WITH THE KIT

1. Micropipettes have to be calibrated to deliver the correct volume required by the assay and must be submitted to regular decontamination (household alcohol, 10% solution of bleach, hospital grade disinfectants) of those parts that could accidentally come in contact with the sample. They should also be regularly maintained in order to show a precision of 1% and a trueness of +/-2%. Decontamination of spills or residues of kit components should also be carried out regularly.
2. The ELISA incubator has to be set at +37°C (tolerance of +/- 0.5°C) and regularly checked to ensure the correct temperature is maintained. Both dry incubators and water baths are suitable for the incubations, provided that the instrument is validated for the incubation of ELISA tests.
3. The **ELISA washer** is extremely important to the overall performances of the assay. The washer must be carefully validated in advance, checked for the delivery of the right dispensation volume and regularly submitted to maintenance according to the manufacturer's instructions for use. In particular the washer, at the end of the daily workload, has to be extensively cleaned out of salts with deionized water. Before use, the washer has to be extensively primed with the diluted Washing Solution. The instrument weekly has to be submitted to decontamination according to its manual (NaOH 0.1 M decontamination suggested).
5 washing cycles (aspiration + dispensation of 350ul/well of washing solution + 20 sec soaking = 1 cycle) are sufficient to ensure the assay with the declared performances. If soaking is not possible add one more cycle of washing.
An incorrect washing cycle or salt-blocked needles are the major cause of false positive reactions.
4. Incubation times have a tolerance of ±5%.
5. The ELISA microplate reader has to be equipped with a reading filter of 450nm and with a second filter of 620-630nm, mandatory for blanking purposes. Its standard performances should be (a) bandwidth ≤ 10 nm; (b) absorbance range from 0 to ≥ 2.0; (c) linearity to ≥ 2.0; repeatability ≥ 1%. Blanking is carried out on the well identified in the section "Assay Procedure". The optical

system of the reader has to be calibrated regularly to ensure that the correct optical density is measured. It should be regularly maintained according to the manufacturer 's instructions.

6. When using an ELISA automated work station, all critical steps (dispensation, incubation, washing, reading, data handling) have to be carefully set, calibrated, controlled and regularly serviced in order to match the values reported in the section "Internal Quality Control" . The assay protocol has to be installed in the operating system of the unit and validated as for the washer and the reader. In addition, the liquid handling part of the station (dispensation and washing) has to be validated and correctly set. Particular attention must be paid to avoid carry over by the needles used for dispensing and for washing. This must be studied and controlled to minimize the possibility of contamination of adjacent wells. The use of ELISA automated work stations is recommended when the number of samples to be tested exceed 20-30 units per run.
7. Dia.Pro's customer service offers support to the user in the setting and checking of instruments used in combination with the kit, in order to assure compliance with the requirements described. Support is also provided for the installation of new instruments to be used with the kit.

L. PRE ASSAY CONTROLS AND OPERATIONS

1. Check the expiration date of the kit printed on the external label (primary container). Do not use if expired.
2. Check that the liquid components are not contaminated by visible particles or aggregates.
3. Check that the Chromogen (TMB) is colourless or pale blue by aspirating a small volume of it with a sterile plastic pipette.
4. Check that no breakage occurred in transportation and no spillage of liquid is present inside the box (primary container). Check that the aluminium pouch, containing the microplate, is not punctured or damaged.
5. Dissolve the content of the lyophilised Control Serum as reported in the proper section.
6. Dilute all the content of the 20x concentrated Wash Solution as described above.
7. Allow all the other components to reach room temperature (about 1 hr) and then mix gently on vortex all liquid reagents.
8. Set the ELISA incubator at +37°C and prepare the ELISA washer by priming with the diluted washing solution, according to the manufacturers instructions. Set the right number of washing cycles reported in the specific section.
9. Check that the ELISA reader is turned on or ensure it will be turned on at least 20 minutes before reading.
10. If using an automated work station, turn on, check settings and be sure to use the right assay protocol.
11. Check that the micropipettes are set to the required volume.
12. Check that all the other equipment is available and ready to use.
13. In case of problems, do not proceed further with the test and advise the supervisor.

M. ASSAY PROCEDURE

The assay has to be carried out according to what reported below, taking care to maintain the same incubation time for all the samples in testing.
The kit may be used for quantitative and qualitative determinations as well.

M1. QUANTITATIVE DETERMINATION:

Automated assay:

In case the test is carried out automatically with an ELISA system, we suggest to make the instrument aspirate 1000 µl Sample Diluent and then 10 µl sample (1:101 dilution factor).

The whole content is then dispensed into a properly defined dilution tube. Before the next sample is aspirated, needles have to be duly washed to avoid any cross-contamination among samples. When all the samples have been diluted make the instrument dispense 100 µl samples into the proper wells of the microplate.

This procedure may be carried out also in two steps of dilutions of 1:10 each (90 µl Sample Diluent + 10 µl sample) into a second dilution platform. Make then the instrument aspirate first 100 µl Sample Diluent, then 10 µl liquid from the first dilution in the platform and finally dispense the whole content in the proper well of the assay microplate.

Do not dilute Calibrators and the dissolved Control Serum as they are ready to use.

Dispense 100 µl calibrators/control in the appropriate calibration/control wells.

For the next operations follow the operative instructions reported below for the Manual Assay.

It is strongly recommended to check that the time lap between the dispensation of the first and the last sample will be calculated by the instrument and taken into consideration by delaying the first washing operation accordingly.

Manual assay:

1. Dilute samples 1:101 into a properly defined dilution tube (example: 1000 µl Sample Diluent + 10 µl sample). Do not dilute the Calibration Set as calibrators are ready to use. Mix carefully all the liquid components on vortex and then proceed as described below.
2. Place the required number of microwells in the microwell holder. Leave the A1 and B1 empty for the operation of blanking.
3. Dispense 100 µl of Calibrators and 100 µl Control Serum in duplicate. Then dispense 100 µl of diluted samples in each properly identified well.
4. Incubate the microplate for **60 min at +37°C**.

Important note: Strips have to be sealed with the adhesive sealing foil, supplied, only when the test is carried out manually. Do not cover strips when using ELISA automatic instruments.

5. Wash the microplate with an automatic washer by delivering and aspirating 350 µl/well of diluted washing solution as reported previously (section I.3).
6. Pipette 100 µl Enzyme Conjugate into each well, except A1+B1 blanking wells, and cover with the sealer. Check that this red coloured component has been dispensed in all the wells, except A1 and B1.

Important note: Be careful not to touch the plastic inner surface of the well with the tip filled with the Enzyme Conjugate. Contamination might occur.

7. Incubate the microplate for **60 min at +37°C**.
8. Wash microwells as in step 5.
9. Pipette 100 µl Chromogen/Substrate mixture into each well, the blank wells A1 and B1 included. Then incubate the microplate at **room temperature (18-24°C) for 20 minutes**.

Important note: Do not expose to strong direct illumination. High background might be generated.

10. Pipette 100 µl Sulphuric Acid to stop the enzymatic reaction into all the wells using the same pipetting sequence as in step 9. Addition of acid will turn the positive calibrators, the control serum and the positive samples from blue to yellow.
11. Measure the colour intensity of the solution in each well, as described in section I.5, at 450nm filter (reading) and at 620-630nm (background subtraction, mandatory), blanking the instrument on A1 or B1 or both.

M2. QUALITATIVE DETERMINATION

If only a qualitative determination is required, proceed as described below:

Automated assay:

Proceed as described in section M1.

Manual assay:

1. Dilute samples 1:101 into a properly defined dilution tube (example: 1000 µl Sample Diluent + 10 µl sample). Do not dilute the Calibration Set as calibrators are ready to use. Mix carefully all the liquid components on vortex and then proceed as described below.
2. Place the required number of Microwells in the microwell holder. Leave A1 well empty for the operation of blanking.
3. Dispense 100 µl of Calibrator 0 arbU/ml and Calibrator 5 arbU/ml in duplicate and Calibrator 100 arbU/ml in single. Then dispense 100 µl of diluted samples in each properly identified well.
4. Incubate the microplate for **60 min at +37°C**.

Important note: Strips have to be sealed with the adhesive sealing foil, supplied, only when the test is carried out manually. Do not cover strips when using ELISA automatic instruments.

5. Wash the microplate with an automatic washer by delivering and aspirating 350 µl/well of diluted washing solution as reported previously (section I.3).
6. Pipette 100 µl Enzyme Conjugate into each well, except the A1 well, and cover with the sealer. Check that this red coloured component has been dispensed in all the wells, except A1.

Important note: Be careful not to touch the plastic inner surface of the well with the tip filled with the Enzyme Conjugate. Contamination might occur.

7. Incubate the microplate for **60 min at +37°C**.
8. Wash microwells as in step 5.
9. Pipette 100 µl Chromogen/Substrate mixture into each well, the blank well included. Then incubate the microplate at **room temperature (18-24°C) for 20 minutes**.

Important note: Do not expose to strong direct illumination. High background might be generated.

10. Pipette 100 µl Sulphuric Acid into all the wells using the same pipetting sequence as in step 9. Addition of acid will turn the positive calibrators, the control serum and the positive samples from blue to yellow.
11. Measure the colour intensity of the solution in each well, as described in section I.5, at 450nm filter (reading) and at 620-630nm (background subtraction, mandatory), blanking the instrument on A1.

General Important notes:

1. Ensure that no finger prints are present on the bottom of the microwell before reading. Finger prints could generate false positive results on reading.
2. Reading has to be carried out just after the addition of the Stop Solution and anyway not any longer than 20 minutes after its addition. Some self oxidation of the chromogen can occur leading to high background.

N. ASSAY SCHEME

Method	Operations
Calibrators & Control (*)	100 µl
Samples diluted 1:101	100 µl
1 st incubation	60 min
Temperature	+37°C

Wash step	n° 5 cycles with 20" of soaking OR n° 6 cycles without soaking
Enzyme conjugate	100 µl
2 nd incubation	60 min
Temperature	+37°C
Wash step	n° 5 cycles with 20" of soaking OR n° 6 cycles without soaking
TMB/H ₂ O ₂	100 µl
3 rd incubation	20 min
Temperature	r.t.
Sulphuric Acid	100 ul
Reading OD	450nm / 620-630nm

(* Important Notes:

- The Control Serum (CS) it does not affect the test's results calculation.
- The Control Serum (CS) used only if a laboratory internal quality control is required by the Management.

An example of dispensation scheme for Quantitative Analysis is reported below:

Microplate

	1	2	3	4	5	6	7	8	9	10	11	12
A	BLK	CAL4	S 1									
B	BLK	CAL4	S 2									
C	CAL1	CAL5	S 3									
D	CAL1	CAL5	S 4									
E	CAL2	CAL6	S 5									
F	CAL2	CAL6	S 6									
G	CAL3	CS(*)	S 7									
H	CAL3	CS(*)	S 8									

Legenda: BLK = Blank CAL = Calibrator
CS(*) = Control Serum - Not mandatory S = Sample

An example of dispensation scheme in qualitative assays is reported below:

Microplate

	1	2	3	4	5	6	7	8	9	10	11	12
A	BLK	S 3	S 11									
B	CAL1	S 4	S 12									
C	CAL1	S 5	S 13									
D	CAL2	S 6	S 14									
E	CAL2	S 7	S 15									
F	CAL6	S 8	S 16									
G	S1	S 9	S 17									
H	S2	S 10	S 18									

Legenda: BLK = Blank CAL = Calibrators
S = Sample

O. INTERNAL QUALITY CONTROL

A validation check is carried out on the calibrators any time the kit is used in order to verify whether the performances of the assay are as qualified.

Control that the following data are matched:

Check	Requirements
Blank well	< 0.050 OD450nm/620-630nm value
CAL 1 0 arbU/ml	< 0.150 mean OD450nm/620-630nm value after blanking coefficient of variation < 30%
CAL 2 5 arbU/ml	OD450nm > OD450nm/620-630nm CAL1 + 0.100
CAL 6 100 arbU/ml	OD450nm/620-630nm > 1.000

If the results of the test match the requirements stated above, proceed to the next section.

If they do not, do not proceed any further and operate as follows:

Problem	Check
Blank well > 0.050 OD450nm/620-630nm	1. that the Chromogen/Sustrate solution has not got contaminated during the assay
CAL 1 0 arbU/ml > 0.150 OD450nm/620-630nm after blanking coefficient of variation > 30%	1. that the washing procedure and the washer settings are as validated in the pre qualification study; 2. that the proper washing solution has been used and the washer has been primed with it before use; 3. that no mistake has been done in the assay procedure (dispensation of a positive calibrator instead of the negative one); 4. that no contamination of the negative calibrator or of their wells has occurred due spills of positive samples or the enzyme conjugate; 5. that micropipettes haven't got contaminated with positive samples or with the enzyme conjugate 6. that the washer needles are not blocked or partially obstructed.
CAL 2 5 arbU/ml OD450nm/620-630nm < OD450nm/620-630nm CAL1 + 0.100	1. that the procedure has been correctly executed; 2. that no mistake has been done in its distribution (ex.: dispensation of a wrong calibrator instead); 3. that the washing procedure and the washer settings are as validated in the pre qualification study; 4. that no external contamination of the calibrator has occurred.
CAL 6 100 arbU/ml < 1.000 OD450nm/620-630nm	1. that the procedure has been correctly executed; 2. that no mistake has been done in its distribution (dispensation of a wrong calibrator instead); 3. that the washing procedure and the washer settings are as validated in the pre qualification study; 4. that no external contamination of the positive control has occurred.

Should one of these problems have happened, after checking, report to the supervisor for further actions.

**** Note:**

If Control Serum has used, verify the following data:

Check	Requirements
Control Serum	Mean OD450nm/620-630nm CAL 4 ± 20%

If the results of the test doesn't match the requirements stated above, operate as follows:

Problem	Check
Control Serum Different from expected value	1. that the procedure has been correctly executed; 2. that no mistake has been done in its distribution (dispensation of a wrong calibrator instead); 3. that the washing procedure and the washer settings are as validated in the pre qualification study; 4. that no external contamination of the control serum has occurred.

Anyway, if all other parameters (Blank, CAL1, CAL2, CAL6), match the established requirements, the test may be considered valid.


P. RESULTS

P.1 Quantitative method

If the test turns out to be valid, use for the quantitative method an approved curve fitting program to draw the calibration curve from the values obtained by reading at OD450nm/620-630nm (4-parameters interpolation is suggested). Then on the calibration curve calculate the concentration of anti Herpes Simplex Virus IgG antibody in samples.

An example of Calibration curve is reported in the next page.

Example of Calibration Curve :

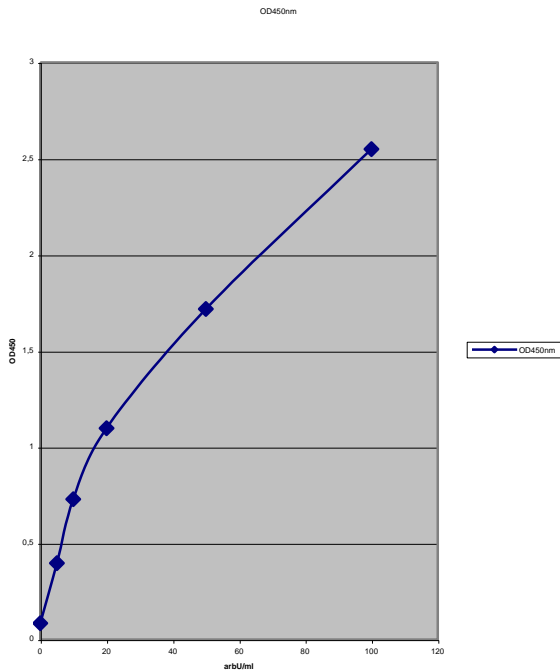

Important Note:

Do not use the calibration curve above to make calculations.

P.2 Qualitative method

In the qualitative method, calculate the mean OD450nm/620-630nm values for the Calibrators 0 and 5 arbU/ml and then check that the assay is valid.

Example of calculation:

The following data must not be used instead of real figures obtained by the user.

Calibrator 0 arbU/ml: 0.020 – 0.024
 Mean Value: 0.022 OD450nm/620-630nm
 Lower than 0.150 – Accepted

Calibrator 5 arbU/ml: 0.350 – 0.370
 Mean Value: 0.360 OD450nm/620-630nm
 Higher than Cal 0 + 0.100 – Accepted

Calibrator 100 arbU/ml: 2.245 OD450nm/620-630nm
 Higher than 1.000 – Accepted

Q. INTERPRETATION OF RESULTS

Samples with a concentration lower than 5 arbU/ml are considered negative for anti HSV IgG antibody.

Samples with a concentration higher than 5 arbU/ml are considered positive for anti HSV IgG antibody.

Particular attention in the interpretation of results has to be used in the follow-up of pregnancy for a primary infection of HSV due to the risk of neonatal malformations.

Important notes:

1. Interpretation of results should be done under the supervision of the laboratory supervisor to reduce the risk of judgment errors and misinterpretations.
2. When test results are transmitted from the laboratory to another facility, attention must be paid to avoid erroneous data transfer.
3. In the follow-up of pregnancy for HSV infection a positive result (presence of IgG antibody > 5 arbU/ml) should be confirmed to ruled out the risk of a false positive result and a false definition of protection.

R. PERFORMANCES

1. Limit of detection

The limit of detection of the assay has been calculated by means of an internal Gold Standard in absence of an international preparation to refer to.

The limit of detection has been calculated as mean OD450nm/620-630nm Calibrator 0 arbU/ml + 5 SD.

The table below reports the mean OD450nm/620-630nm values of this standard when diluted in negative plasma and then examined in the assay for three lots.

Mean OD450nm/620-630nm values (n = 2)

IgG arbU/ml	HSV.G.PU Lot. 0203/2	HSV.G Lot. 0403/M	HSV.G.PU Lot. 0603
0	0.043	0.085	0.091
5	0.381	0.397	0.427
10	0.694	0.729	0.786
20	1.076	1.099	1.097
50	1.550	1.719	1.692
100	2.396	2.549	2.478

The assay shows a limit of detection far better than 5 arbU/ml.

In addition the preparation code Accurun n° 150, produced by Boston Biomedica Inc., BBI, USA, was tested in dilutions to determine the limit of its detection and provide a further value of analytical sensitivity

Mean OD450nm/620-630nm values (n = 2)

Dilution	HSV.G.PU Lot. 0203/2	HSV.G Lot. 0403/M	HSV.G.PU Lot. 0603
1 X	1.694	1.719	1.708
2 X	1.085	1.117	1.100
4 X	0.730	0.751	0.744
8 X	0.446	0.464	0.453
16 X	0.301	0.314	0.306
32 X	0.150	0.165	0.158
0 arbU/ml	0.043	0.085	0.066
5 arbU/ml	0.381	0.397	0.395

2. Diagnostic sensitivity:

The diagnostic sensitivity has been tested in a performance evaluation study on panels of samples classified positive by a kit US FDA approved. Positive samples from different stage of HSV infection were tested.

The value, obtained from the analysis of more than 300 specimens, has been > 98%.

In addition the Performance panel PTH 201, supplied by BBI, was evaluated with the kit against a reference FDA approved kit.

BBI Panel PTH 201 (Performance)

Panel ID #	Dia.Pro OD450nm/620-630nm	Kit S/Co	REF HSV1 S/Co	REF HSV2 S/Co
01	1.064	2.7	3.5	1.6
02	2.525	6.4	2.9	4.4
03	0.860	2.1	1.0	1.1
04	2.391	6.0	4.4	4.1
05	1.793	4.5	4.0	2.2
06	1.093	2.8	0.8	1.4
07	0.801	2.0	0.9	1.2
08	2.180	5.5	2.9	3.9
09	2.086	5.3	4.6	3.4
10	0.029	0.1	0.3	0.3
11	1.900	4.8	3.8	2.7
12	0.995	2.5	2.1	2.3
13	1.833	4.6	2.4	3.3
14	0.153	0.4	0.4	0.5
15	2.130	5.4	4.7	3.6
16	1.320	3.3	1.9	2.7
17	3.008	7.6	4.6	5.6
18	1.042	2.6	2.8	1.6
19	0.097	0.2	0.3	0.3
20	0.414	1.0	0.6	0.8
21	1.682	4.2	3.3	2.2
22	2.364	6.0	5.1	4.1
23	1.926	4.9	4.3	2.2
24	1.556	4.0	1.6	2.5
25	2.372	6.0	5.1	3.7

Note: Cut-Off = 5 arbU/ml = 0.395

3. Diagnostic specificity:

The diagnostic specificity has been determined in the same study on panels of negative samples from not infected individuals, classified negative with a kit US FDA approved.

Both plasma, derived with different standard techniques of preparation (citrate, EDTA and heparin), and sera have been used to determine the value of specificity.

Frozen specimens have been tested, as well, to check for interferences due to collection and storage.

No interference was observed.

Potentially interfering samples derived from patients with different pathologies (mostly ANA, AMA and RF positive) and from pregnant women were tested.

No crossreaction was observed.

An overall value > 98% of specificity was found when examined on more than 100 specimens.

3. Precision:

It has been calculated on the Calibrator 5 arbU/ml, considered the cut-off of the assay, examined in 16 replicates in three separate runs for three lots.

Results are reported as follows:

HSV: lot 0603/2

Mean values	1st run	2nd run	3 rd run	Average value
OD450nm/620-630nm	0.450	0.438	0.449	0.446
Std.Deviation	0.020	0.021	0.026	0.022
CV %	4.4	4.8	5.7	5.0

HSV: lot 0603

Mean values	1st run	2nd run	3 rd run	Average value
OD450nm/620-630nm	0.449	0.441	0.453	0.448
Std.Deviation	0.024	0.024	0.029	0.026
CV %	5.4	5.4	6.5	5.8

HSV: Lot 0403/M

Mean values	1st run	2nd run	3 rd run	Average value
OD450nm/620-630nm	0.405	0.406	0.405	0.405
Std.Deviation	0.027	0.031	0.030	0.029
CV %	6.6	7.6	7.4	7.2

The variability shown in the tables above did not result in sample misclassification.

5. Accuracy

The assay accuracy has been checked by the dilution and recovery tests. Any "hook effect", underestimation likely to happen at high doses of analyte, was ruled out up to 500 IU/ml.

S. LIMITATIONS OF THE PROCEDURE

Bacterial contamination or heat inactivation of the specimen may affect the absorbance values of the samples with consequent alteration of the level of the analyte.

Frozen samples containing fibrin particles or aggregates after thawing may generate some false results.

This test is suitable only for testing single samples and not pooled ones.

Diagnosis of an infectious disease should not be established on the basis of a single test result. The patient's clinical history, symptomatology, as well as other diagnostic data should be considered.

REFERENCES

- Engvall E. and Perlmann P.. J.Immunochemistry 8: 871-874, 1971
- Engvall E. and Perlmann P.. J.Immunol.. 109: 129-135, 1971
- Remington J.S. and Klein J.O.. (1996) In "Infectious diseases of fetus and newborn infant". Sanders, Philadelphia, London, Toronto.
- Volk W.A. (1982) In "essential of Medical Microbiology". 2nd ed., pp 729, G.B. Lippincott Co. Philadelphia, New York, S.Josè, Toronto.
- Leinikki P.O. et al.. J.Clin.Microbiol.. 8:418, 1978
- Piroid E. et al.. Révue Méd.Vet.. 131:25, 1980.
- Vaheri A. et al.. J.Med.Virol.. 5:171, 1980.
- Vejtorp M. et al.. Acta Path.Microbiol.Scand.. 88:349, 1980.
- Voller A. et al.. Brit.J.Exp.Pathol.. 56:338, 1975

All the IVD Products manufactured by the company are under the control of a certified Quality Management System in compliance with ISO 13485 rule. Each lot is submitted to a quality control and released into the market only if conforming with the EC technical specifications and acceptance criteria.

Manufacturer:
Dia.Pro Diagnostic Bioprobes S.r.l.
Via G. Carducci n° 27 – Sesto San Giovanni (MI) – Italy



HSV_{1&2} IgG

**Ensayo inmunoenzimático (ELISA) para la
determinación cualitativa/cuantitativa de
anticuerpos IgG al Virus
Herpes Simple tipos 1 y 2
en suero y plasma humanos**

- Uso exclusivo para diagnóstico "in vitro" -



DIA.PRO

**Diagnostic Bioprobes Srl
Via G. Carducci n° 27
20099 Sesto San Giovanni
(Milán) - Italia**

Teléfono +39 02 27007161

Fax +39 02 44386771

e-mail: info@diapro.it

REF HSVG.CE
96 pruebas

HSV IgG

A. OBJETIVO DEL ESTUCHE.

Ensayo inmunoenzimático (ELISA) para la determinación cualitativa/cuantitativa de anticuerpos al Virus Herpes Simple tipos 1 y 2, en plasma y suero humanos. Uso exclusivo para diagnóstico "in vitro".

B. INTRODUCCIÓN.

Los Virus del Herpes Simple tipos 1 (HSV1) y 2 (HSV2) son grandes y complejos virus ADN que inducen la síntesis de varias proteínas durante la infección, poseen un alto número de determinantes de reactividad cruzada y pocas secuencias tipo específicas.

La mayor parte de las infecciones herpéticas primarias y recurrentes son causadas por HSV2, mientras que aquellas infecciones no asociadas a los genitales son causadas fundamentalmente por HSV1.

La detección de anticuerpos IgG e IgM específicos al virus, es importante en el diagnóstico de las infecciones agudas/primarias, así como en las reactivaciones de una infección latente, en ausencia de síntomas clínicos evidentes.

En individuos aparentemente sanos y durante el embarazo, pueden aparecer infecciones asintomáticas debidas a HSV. En pacientes inmunocomprometidos se pueden presentar severas infecciones herpéticas, donde la enfermedad evoluciona hacia patologías críticas.

La determinación de anticuerpos específicos al virus constituye un elemento importante para el seguimiento de pacientes en grupos de riesgo, así como para el monitoreo de las infecciones severas y agudas.

C. PRINCIPIOS DEL ENSAYO.

Las microplacas están recubiertas con antígenos nativos de HSV1 y HSV2, inactivados.

Primeramente se añaden a la placa las muestras diluidas, quedando capturados por los antígenos de la fase sólida los anticuerpos IgG al HSV presentes en la muestra.

Previo lavado, en la 2^{da} incubación, los anticuerpos IgG inmovilizados se detectan mediante anticuerpos policlonales específicos anti-IgG humanos conjugados con Peroxidasa (HRP).

Luego de la adición del sustrato cromogénico y producto de la combinación del mismo con la enzima capturada en la fase sólida, se genera una señal coloreada proporcional a la cantidad de anticuerpos IgG al HSV, presentes en la muestra. La determinación cuantitativa de anticuerpos IgG, se realiza con ayuda de una Curva de Calibración construida contra un Gold Standard interno.

D. COMPONENTES.

Cada estuche contiene reactivos suficientes para realizar 96 pruebas.

1. Microplaca: **MICROPLATE**

12 tiras de 8 pocillos recubiertos con antígenos nativos de HSV1 y HSV2, inactivados por radiaciones UV, en presencia de proteínas de bovino.

Las placas están en una bolsa sellada con desecante. Se deben poner las mismas a temperatura ambiente antes de abrirlas, sellar las tiras sobrantes en la bolsa con el desecante y almacenar entre 2 y 8°C.

2. Curva de Calibración: **CAL N° ...**

Listo para el uso y curva con código estándar de color, elaborada a partir de plasma humano positivo a IgG anti-HSV con rangos:

4ml CAL1 = 0 arbU/ml

4ml CAL2 = 5 arbU/ml

2ml CAL3 = 10 arbU/ml

2ml CAL4 = 20 arbU/ml

2ml CAL5 = 50 arbU/ml

4ml CAL6 = 100 arbU/ml.

Los estándares han sido calibrados en unidades arbitrarias contra un Gold Standard interno (o IGS).

Contiene proteínas séricas humanas, caseína 2%, tampón citrato sódico 10 mM pH 6.0 +/-0.1, 0.1% de Tween 20, así como azida sódica 0.09% y P como preservativos. Los estándares son de color azul.

3. Suero Control: **CONTROL ...ml**

1 vial. Liofilizado. Contiene proteínas del suero fetal bovino, anticuerpos humanos IgG contra HSV a una concentración aproximada de 10 arbU/ml \pm 20%, además de sulfato de gentamicina 0.2 mg/ml y ProClin 300 0.045% como preservativos.

Nota: El volumen necesario para disolver el contenido del frasco varía en cada lote. Se recomienda usar el volumen indicado en la etiqueta.

4. Tampón de Lavado Concentrado: **WASHBUF 20X**

1x60ml/botella. Solución concentrada 20x. Una vez diluida, la solución de lavado contiene tampón fosfato 10 mM a pH 7.0 +/-0.2, Tween 20 al 0.05% y ProClin 300 al 0.045%.

5. Conjugado: **CONJ**

2x8ml/vial. Solución lista para el uso. Codificado con el color rojo. Contiene anticuerpos policlonales anti-IgG humanos conjugados con Peroxidasa (HRP), BSA 5%, tampón Tris 10 mM pH 6.8 +/-0.1, además de sulfato de gentamicina 0.02% y ProClin 300 0.045% como preservativos y 0.01% de colorante rojo.

6. Cromógeno/Sustrato: **SUBS TMB**

1x16ml/vial. Contiene una solución tamponada citrato-fosfato 50 mM pH 3.5-3.8, dimetilsulfóxido 4%, tetra-metil-benzidina (TMB) 0.03% y peróxido de hidrógeno (H₂O₂) 0.02%.

Nota: Evitar la exposición a la luz, ya que la sustancia es fotosensible.

6. Ácido Sulfúrico: **H₂SO₄ 0.3M**

1x15ml/vial. Contiene solución de H₂SO₄ 0.3M H315, H319; P280, P302+P352, P332+P313, P305+P351+P338, P337+P313, P362+P363).

8. Diluyente de muestras: **DILSPE**

2x60ml/vial. Contiene 2% de caseína, tampón citrato sódico 10 mM pH 6.0 +/-0.1, 0.1% de Tween 20, así como azida sódica 0.09% y ProClin 300 0.045% como preservativos. El reactivo está codificado con el color azul.

9. Sellador adhesivo, n° 2

10. Manual de instrucciones, n° 1

E. MATERIALES NECESARIOS NO SUMINISTRADOS.

1. Micropipetas calibradas (1000µl, 100µl y 10µl) y puntas plásticas desechables.
2. Agua de calidad EIA (bidestilada o desionizada, tratada con carbón para remover químicos oxidantes usados como desinfectantes).
3. Timer con un rango de 60 minutos como mínimo.
4. Papel absorbente.

5. Incubador termostático de microplacas ELISA, calibrado (en seco o húmedo) fijo a 37°C (tolerancia+/-0.5°C).
6. Lector calibrado de microplacas de ELISA con filtros de 450nm (lectura) y de 620-630 nm.
7. Lavador calibrado de microplacas ELISA.
8. Vórtex o similar.

F. ADVERTENCIAS Y PRECAUCIONES.

1. El estuche debe ser usado por personal técnico adecuadamente entrenado, bajo la supervisión de un doctor responsable del laboratorio.
2. Todas las personas encargadas de la realización de las pruebas deben llevar las ropas protectoras adecuadas de laboratorio, guantes y gafas. Evitar el uso de objetos cortantes (cuchillas) o punzantes (agujas). El personal debe ser adiestrado en procedimientos de bioseguridad, según ha sido recomendado por el Centro de Control de Enfermedades de Atlanta, Estados Unidos, y publicado por el Instituto Nacional de Salud: "Biosafety in Microbiological and Biomedical Laboratories", ed.1984.
3. Todo el personal involucrado en el manejo de muestras debe estar vacunado contra HBV y HAV, para lo cual existen vacunas disponibles, seguras y eficaces.
4. Se debe controlar el ambiente del laboratorio para evitar la contaminación de los componentes con polvo o agentes microbianos cuando se abran los estuches, así como durante la realización del ensayo. Evitar la exposición del sustrato a la luz y las vibraciones de la mesa de trabajo durante el ensayo.
5. Conservar el estuche a temperaturas entre 2-8 °C, en un refrigerador con temperatura regulada o en cámara fría.
6. No intercambiar reactivos de diferentes lotes ni tampoco de diferentes estuches.
7. Comprobar que los reactivos no contienen precipitados ni agregados en el momento del uso. De darse el caso, informar al supervisor para realizar el procedimiento pertinente.
8. Evitar contaminación cruzada entre muestras de suero/plasma usando puntas desechables y cambiándolas luego de cada uso. No reutilizar puntas desechables.
9. Evitar contaminación cruzada entre los reactivos del estuche usando puntas desechables y cambiándolas luego de cada uso. No reutilizar puntas desechables.
10. No usar el producto después de la fecha de caducidad indicada en el estuche e internamente en los reactivos. Según estudios realizados, no se ha detectado pérdida relevante de actividad en estuches abiertos, en uso por un período de hasta 6 meses.
11. Tratar todas las muestras como potencialmente infecciosas. Las muestras de suero humano deben ser manipuladas al nivel 2 de bioseguridad, según ha sido recomendado por el Centro de Control de Enfermedades de Atlanta, Estados Unidos y publicado por el Instituto Nacional de Salud: "Biosafety in Microbiological and Biomedical Laboratories", ed.1984.
12. Se recomienda el uso de material plástico desechable para la preparación de las soluciones de lavado y para la transferencia de los reactivos a los diferentes equipos automatizados a fin de evitar contaminaciones.
13. Los desechos producidos durante el uso del estuche deben de ser eliminados según lo establecido por las directivas nacionales y las leyes relacionadas con el tratamiento de los residuos químicos y biológicos de laboratorio. En particular, los desechos líquidos provenientes del proceso de lavado deben ser tratados como potencialmente infecciosos y deben ser inactivados. Se recomienda la inactivación con lejía al 10% de 16 a 18 horas o el uso de la autoclave a 121°C por 20 minutos.
14. En caso de derrame accidental de algún producto, se debe utilizar papel absorbente embebido en lejía y posteriormente en agua. El papel debe eliminarse en

contenedores designados para este fin en hospitales y laboratorios.

15. El ácido sulfúrico es irritante. En caso de derrame, se debe lavar la superficie con abundante agua.
16. Otros materiales de desecho generados durante la utilización del estuche (por ejemplo: puntas usadas en la manipulación de las muestras y controles, microplacas usadas) deben ser manipuladas como fuentes potenciales de infección de acuerdo a las directivas nacionales y leyes para el tratamiento de residuos de laboratorio.

G. MUESTRA: PREPARACIÓN Y RECOMENDACIONES.

1. Extraer la sangre asépticamente por punción venosa y preparar el suero o plasma según las técnicas estándar de los laboratorios de análisis clínico. No se ha detectado que el tratamiento con citrato, EDTA o heparina afecte las muestras.
2. Las muestras deben estar identificadas claramente mediante código de barras o nombres, a fin de evitar errores en los resultados. Cuando el estuche se emplea para el pesquaje en unidades de sangre, se recomienda el uso del código de barras.
3. Las muestras hemolizadas (color rojo) o hiperlipémicas (aspecto lechoso) deben ser descartadas para evitar falsos resultados, al igual que aquellas donde se observe la presencia de precipitados, restos de fibrina o filamentos microbianos.
4. El suero y el plasma pueden conservarse a una temperatura entre +2° y +8°C en tubos de recolección principales hasta cinco días después de la extracción. No congelar tubos de recolección principales. Para periodos de almacenamiento más prolongados, las muestras de plasma o suero, retiradas cuidadosamente del tubo de extracción principal, pueden almacenarse congeladas a -20°C al menos 12 meses. Evitar congelar/descongelar cada muestra más de una vez, ya que pueden generarse partículas que podrían afectar al resultado de la prueba.
5. Si hay presencia de agregados, la muestra se puede aclarar mediante centrifugación a 2000 rpm durante 20 minutos o por filtración con un filtro de 0,2-0,8 micras.

H. PREPARACIÓN DE LOS COMPONENTES Y PRECAUCIONES.

Según estudios realizados, no se ha detectado pérdida relevante de actividad en estuches abiertos, en uso por un período de hasta 3 meses.

Microplacas:

Dejar la microplaca a temperatura ambiente (aprox. 1 hora) antes de abrir el envase. Compruebe que el desecante no esté de un color verde oscuro, lo que indicaría un defecto de fabricación. De ser así, debe solicitar el servicio de Dia.Pro: atención al cliente.

Las tiras de pocillos no utilizadas, deben guardarse herméticamente cerradas en la bolsa de aluminio con el desecante a 2-8°C. Una vez abierto el envase, las tiras sobrantes, se mantienen estables hasta que el indicador de humedad dentro de la bolsa del desecante cambie de amarillo a verde.

Curva de Calibración:

Listo para el uso. Mezclar bien con la ayuda de un vórtex, antes de usar.

Suero Control:

Añadir al polvo liofilizado el volumen de agua de calidad ELISA indicado en la etiqueta. Dejar disolver totalmente y mezclar suavemente en el vórtex.

Nota: Una vez reconstituida, la solución no es estable. Se recomienda mantenerla congelada en alícuotas a -20°C.

Solución de Lavado Concentrada:

Todo el contenido de la solución concentrada 20x debe diluirse con agua bidestilada y mezclarse suavemente antes de usarse. Durante la preparación evitar la formación de espuma y burbujas, lo que podría influir en la eficiencia de los ciclos de lavado.

Nota: Una vez diluida, la solución es estable por una semana a temperaturas entre +2 y 8°C.

Conjugado:

Listo para el uso. Mezclar bien con un vórtex antes de usar. Evitar posible contaminación del líquido con oxidantes químicos, polvo o microbios. En caso de que deba transferirse el reactivo, usar contenedores de plástico, estériles y desechables, siempre que sea posible.

Cromógeno/ Substrato:

Listo para el uso. Mezclar bien con un vórtex antes de usar. Evitar posible contaminación del líquido con oxidantes químicos, polvo o microbios. Evitar la exposición a la luz, agentes oxidantes y superficies metálicas. En caso de que deba transferirse el reactivo, usar contenedores de plástico, estériles y desechables, siempre que sea posible.

Diluyente de muestras :

Solución lista para el uso. Mezclar bien con un vórtex antes de usar.

Ácido Sulfúrico:

Listo para el uso. Mezclar bien con un vórtex antes de usar. Atención: Irritante (H315, H319; P280, P302+P352, P332+P313, P305+P351+P338, P337+P313, P362+P363).

Leyenda:

Indicación de peligro, Frases H

H315 – Provoca irritación cutánea.

H319 – Provoca irritación ocular grave.

Consejo de prudencia, Frases P

P280 – Llevar guantes/prendas/gafas/máscara de protección.

P302 + P352 – EN CASO DE CONTACTO CON LA PIEL: Lavar con agua y jabón abundantes.

P332 + P313 – En caso de irritación cutánea: Consultar a un médico.

P305 + P351 + P338 – EN CASO DE CONTACTO CON LOS OJOS: Aclarar cuidadosamente con agua durante varios minutos. Quitar las lentes de contacto, si lleva y resulta fácil. Seguir aclarando.

P337 + P313 – Si persiste la irritación ocular: Consultar a un médico.

P362 + P363 – Quitarse las prendas contaminadas y lavarlas antes de volver a usarlas.

secas o baños de agua siempre que estén validados para la incubación de pruebas de ELISA.

- El **lavador ELISA** es extremadamente importante para el rendimiento global del ensayo. El lavador debe ser validado de forma minuciosa previamente, revisado para comprobar que suministra el volumen de dispensación correcto y enviado regularmente a mantenimiento de acuerdo con las instrucciones de uso del fabricante. En particular, deben lavarse minuciosamente las sales con agua desionizada del lavador al final de la carga de trabajo diaria. Antes del uso, debe suministrarse extensivamente solución de lavado diluida al lavador. Debe enviarse el instrumento semanalmente a descontaminación según se indica en su manual (se recomienda descontaminación con NaOH 0.1 M). Para asegurar que el ensayo se realiza conforme a los rendimientos declarados, basta con 5 ciclos de lavado (aspiración + dispensado de 350 µl/pocillo de solución de lavado + 20 segundos de remojo = 1 ciclo). Si no es posible remojar, añadir un ciclo de lavado adicional. Un ciclo de lavado incorrecto o agujas obstruidas con sal son las principales causas de falsas reacciones positivas.
- Los tiempos de incubación deben tener un margen de $\pm 5\%$.
- El lector de microplacas ELISA debe estar provisto de un filtro de lectura de 450nm y, de un segundo filtro de 620-630nm, obligatorio para reducir interferencias en la lectura. El procedimiento estándar debe contemplar: a) Ancho de banda ≤ 10 b) Rango de absorbancia de 0 a ≥ 2.0 , c) Linealidad ≥ 2.0 , reproducibilidad $\geq 1\%$. El blanco se prueba en el pocillo indicado en la sección "Procedimiento del ensayo". El sistema óptico del lector debe ser calibrado periódicamente para garantizar la correcta medición de la densidad óptica, según las normas del fabricante.
- En caso de usar un sistema automatizado de ELISA, los pasos críticos (dispensado, incubación, lavado, lectura, agitación y procesamiento de datos) deben ser cuidadosamente fijados, calibrados, controlados y periódicamente ajustados, para garantizar los valores indicados en la sección "Control de calidad interno". El protocolo del ensayo debe ser instalado en el sistema operativo de la unidad y validado tanto para el lavador como para el lector. Por otro lado, la parte del sistema que maneja los líquidos (dispensado y lavado) debe ser validada y fijada correctamente. Debe prestarse particular atención a evitar el arrastre por las agujas de dispensación y las de lavado, a fin de minimizar la posibilidad de ocurrencia de falsos positivos por contaminación de los pocillos adyacentes por muestras fuertemente reactivas. Se recomienda el uso de sistemas automatizados para el pesquaje en unidades de sangre y cuando la cantidad de muestras supera las 20-30 unidades por ensayo.
- El servicio de atención al cliente en Dia.Pro, ofrece apoyo al usuario para calibrar, ajustar e instalar los equipos a usar en combinación con el estuche, con el propósito de asegurar el cumplimiento de los requerimientos descritos.

I. INSTRUMENTOS Y EQUIPAMIENTO UTILIZADOS EN COMBINACIÓN CON EL ESTUCHE.

- Las micropipetas deben ser calibradas para dispensar correctamente el volumen requerido en el ensayo y sometidas a una descontaminación periódica de las partes que pudieran entrar accidentalmente en contacto con la muestra (etanol 70%, lejía 10%, de calidad de los desinfectantes hospitalarios). Deben además, ser regularmente revisadas para mantener una precisión del 1% y una confiabilidad de $\pm 2\%$. Los residuos de componentes del estuche deben descontaminarse periódicamente.
- La incubadora de ELISA debe ser ajustada a 37°C ($\pm 0.5^\circ\text{C}$) y controlada periódicamente para mantener la temperatura correcta. Pueden emplearse incubadoras

L. OPERACIONES Y CONTROLES PREVIOS AL ENSAYO.

- Compruebe la fecha de caducidad indicada en la parte externa del estuche (envase primario). No usar si ha caducado.
- Compruebe que los componentes líquidos no están contaminados con partículas o agregados visibles.
- Asegúrese de que el cromógeno (TMB) es incoloro o azul pálido, aspirando un pequeño volumen de este con una pipeta estéril de plástico.
- Compruebe que no han ocurrido rupturas ni derrames de líquido dentro de la caja (envase primario) durante el transporte. Asegurarse de que la bolsa de aluminio que contiene la microplaca no esté rota o dañada.
- Disolver el Suero Control como se ha descrito anteriormente.

- Diluir totalmente la solución de lavado concentrada 20X, como se ha descrito anteriormente.
- Dejar los componentes restantes alcanzar la temperatura ambiente (aprox. 1 hora), mezclar luego suavemente en el vórtex todos los reactivos líquidos.
- Ajustar la incubadora de ELISA a 37°C y cebar el lavador de ELISA utilizando la solución de lavado, según las instrucciones del fabricante. Fijar el número de ciclos de lavado según se indica en la sección específica.
- Comprobar que el lector de ELISA esté encendido al menos 20 minutos antes de realizar la lectura.
- En caso de trabajar automáticamente, encender el equipo y comprobar que los protocolos estén correctamente programados.
- Comprobar que las micropipetas estén fijadas en el volumen requerido.
- Asegurarse de que el equipamiento a usar esté en perfecto estado, disponible y listo para el uso.
- En caso de surgir algún problema, se debe detener el ensayo y avisar al supervisor.

M. PROCEDIMIENTO DEL ENSAYO.

El ensayo debe realizarse según las instrucciones que siguen a continuación, es importante mantener en todas las muestras el mismo tiempo de incubación.

El estuche puede emplearse tanto para la determinación cuantitativa como cualitativa de anticuerpos.

M1. DETERMINACIÓN CUANTITATIVA:

Ensayo automatizado:

En el caso de que el ensayo se realice de manera automatizada con un sistema ELISA, se recomienda programar el equipo para aspirar 1000µl de Diluyente de Muestras, y posteriormente 10µl de muestra (factor de dilución 1:101).

La mezcla debe ser dispensada cuidadosamente en un tubo de dilución. Antes de aspirar la muestra siguiente, las agujas deben lavarse debidamente para evitar cualquier contaminación cruzada entre las muestras. Cuando todas las muestras han sido diluidas, programar el equipo para dispensar 100 µl de las mismas en los pocillos correspondientes.

Este procedimiento puede realizarse en dos pasos de dilución de 1:10 cada uno (90 µl de Diluyente de Muestras + 10 µl de muestra) en una segunda plataforma de dilución. Programar el equipo para aspirar primeramente 100 µl de Diluyente de Muestras, luego 10 µl de la primera dilución en la plataforma y finalmente dispensar todo el contenido en los pocillos apropiados de la microplaca.

No diluir el Calibrador ni el Suero Control disuelto, ya que están listos para el uso.

Dispensar 100ul de controles/calibrador en los pocillos correspondientes.

Para las operaciones siguientes, consulte las instrucciones que aparecen debajo para el Ensayo Manual.

Es muy importante comprobar que el tiempo entre el dispensado de la primera y la última muestra sea calculado por el instrumento y considerado para los lavados.

Ensayo Manual.

- Diluir las muestras 1:101 en un tubo de dilución apropiado (ejemplo: 1000 de Diluyente de Muestras+10µl de muestra). No diluir el Panel de Calibración, ya que los calibradores están listos para el uso. Mezclar cuidadosamente, con ayuda de un vórtex, todos los componentes líquidos y continuar como se describe a continuación.
- Poner el número de tiras necesarias en el soporte de plástico. Dejar vacíos los pocillos A1 y B1 para el blanco.
- Dispensar 100 µl de Calibradores y 100 µl de Suero Control, por duplicado, luego dispensar 100 ul de cada muestra diluida en su pocillo correspondiente.

- Incubar la microplaca **60 min a +37°C**.

Nota importante: Las tiras se deben sellar con el adhesivo suministrado solo cuando se hace el test manualmente. No sellar cuando se emplean equipos automatizados de ELISA.

- Lavar la microplaca según según se indica en la sección I.3.
- Dispensar 100uL del Conjugado en todos los pocillos, excepto en A1 y B1, luego cubrir con el sellador. Compruebe que este reactivo de color rojo ha sido añadido en todos los pocillos excepto A1 y B1.

Nota importante: Tener cuidado de no tocar la pared interna del pocillo con la punta de la pipeta al dispensar el conjugado. Podría producirse contaminación.

- Incubar la microplaca durante **60 minutos a +37°C**.
- Lavar los pocillos de igual forma que en el paso 5.
- Dispensar 100µl de TMB/H₂O₂ en todos los pocillos, incluidos los del blanco. Controlar que los reactivos han sido correctamente añadidos. Incubar la microplaca durante **20 minutos a temperatura ambiente (18-24°C)**.

Nota importante: No exponer directamente a fuerte iluminación, de lo contrario se generan interferencias.

- Dispensar 100µl de Ácido Sulfúrico en todos los pocillos para detener la reacción enzimática, usar la misma secuencia que en el paso 9. La adición del ácido cambia el color de los calibradores positivos, el suero control y las muestras positivas de azul a amarillo.
- Medir la intensidad del color de la solución en cada pocillo, según se indica en la sección I.5, con un filtro de 450 nm (lectura) y otro de 620-630 nm (substracción del fondo, obligatorio), calibrando el instrumento con el pocillo A1 (blanco y B1 (blanco).

M2. DETERMINACIÓN CUALITATIVA:

Si se requiere solamente un análisis cualitativo, proceda como se indica a continuación.

Ensayo automatizado:

Proceder según la sección M1.

Ensayo Manual.

- Diluir las muestras 1:101 en un tubo de dilución apropiado (ejemplo: 1000 de Diluyente de Muestras+10µl de muestra). No diluir el Panel de Calibración, ya que los calibradores están listos para el uso. Mezclar cuidadosamente, con ayuda de un vórtex, todos los componentes líquidos y continuar como se describe a continuación.
- Poner el número de tiras necesarias en el soporte de plástico. Dejar vacío el pocillo A1 para el blanco.
- Dispensar 100 µl del Calibrador 0 IU/ml y del Calibrador 10 IU/ml, por duplicado y del Calibrador 250 IU/ml sencillo, luego dispensar 100 ul de cada muestra diluida en su pocillo correspondiente.
- Incubar la microplaca **60 min a +37°C**.

Nota importante: Las tiras se deben sellar con el adhesivo suministrado solo cuando se hace el test manualmente. No sellar cuando se emplean equipos automatizados de ELISA.

- Lavar la microplaca con el lavador automático dispensando y aspirando 300ul/pocillo de solución de lavado diluida, según según se indica (section I.3).
- Dispensar 100uL del Conjugado en todos los pocillos, excepto en A1, luego cubrir con el sellador. Compruebe que este reactivo de color rojo ha sido añadido en todos los pocillos excepto A1.

Nota importante: Tener cuidado de no tocar la pared interna del pocillo con la punta de la pipeta al dispensar el conjugado. Podría producirse contaminación.

7. Incubar la microplaca durante **60 minutos a +37°C**.
8. Lavar los pocillos de igual forma que en el paso 5.
9. Dispensar 100µl de TMB/H₂O₂ en todos los pocillos, incluido el del blanco. Controlar que los reactivos han sido correctamente añadidos. Incubar la microplaca durante **20 minutos a temperatura ambiente (18-24°C)**.

Nota importante: No exponer directamente a fuerte iluminación, de lo contrario se generan interferencias.

10. Dispensar 100µl de Ácido Sulfúrico en todos los pocillos para detener la reacción enzimática, usar la misma secuencia que en el paso 9. La adición del ácido cambia el color de los calibradores positivos, el suero control y las muestras positivas de azul a amarillo.
11. Medir la intensidad del color de la solución en cada pocillo, según se indica en la sección I.5, con un filtro de 450 nm (lectura) y otro de 620-630 nm (substracción del fondo, obligatorio), calibrando el instrumento con el pocillo A1 (blanco).

Notas generales importantes:

1. Asegurarse de que no hay impresiones digitales en el fondo de los pocillos antes de leer. Podrían generarse falsos positivos en la lectura.
2. La lectura debe hacerse inmediatamente después de añadir la solución de parada y, en cualquier caso, nunca transcurridos 20 minutos después de su adición. Se podría producir auto oxidación del cromógeno causando un elevado fondo.

N. ESQUEMA DEL ENSAYO.

Método	Operaciones
Calibradores & Control (*)	100 µl
Muestras diluidas 1:101	100 µl
1ª incubación	60 min
Temperatura	+37°C
Lavado	5 ciclos con 20" de remojo o 6 ciclos sin remojo
Conjugado	100 µl
2ª incubación	60 min
Temperatura	+37°C
Lavado	5 ciclos con 20" de remojo o 6 ciclos sin remojo
TMB/H ₂ O ₂	100 µl
3ª incubación	20 min
Temperatura	t.a.*
Ácido Sulfúrico	100 ul
Lectura D.O.	450nm / 620-630nm

t.a.*temperatura ambiente

(*) Notas importantes:

- El suero de control (CS) no afecta al cálculo de los resultados de la prueba.
- El suero de control (CS) se usa solo si la gestión requiere un control interno de calidad del laboratorio.

A continuación se describe un ejemplo del esquema de dispensado en el análisis cuantitativo:

Microplaca

	1	2	3	4	5	6	7	8	9	10	11	12
A	BL	CAL4	M 1									
B	BL	CAL4	M 2									
C	CAL1	CAL5	M 3									
D	CAL1	CAL5	M 4									
E	CAL2	CAL6	M 5									
F	CAL2	CAL6	M 6									
G	CAL3	SC(*)	M 7									
H	CAL3	SC(*)	M 8									

Legenda: BL = Blanco // CAL = Calibradores // M = Muestra
SC(*) = Suero Control - No oligatorio

A continuación se describe un ejemplo del esquema de dispensado en el análisis cualitativo:

Microplaca

	1	2	3	4	5	6	7	8	9	10	11	12
A	BL	M 3	M 11									
B	CAL1	M 4	M 12									
C	CAL1	M 5	M 13									
D	CAL2	M 6	M 14									
E	CAL2	M 7	M 15									
F	CAL5	M 8	M 16									
G	M 1	M 9	M 17									
H	M 2	M 10	M 18									

Legenda: BL = Blanco // CAL = Calibradores // M = Muestra

O. CONTROL DE CALIDAD INTERNO.

Se realiza un grupo de pruebas de validación con los controles cada vez que se usa el estuche para verificar si el performance del ensayo es correcto.

Asegurar el cumplimiento de los siguientes parámetros:

Parámetro	Exigencia
Pocillo Blanco	< 0.050 DO450nm/620-630nm
CAL 1 0 arbU/ml	< 0.150 valor medio DO450nm/620-630nm después de leer el blanco Coeficiente de variación < 30%
CAL 2 5 arbU/ml	DO450nm/620-630nm > DO450nm/620-630nm CAL1 + 0.100
CAL 6 100 arbU/ml	DO450nm/620-630nm > 1.000

Si los resultados del ensayo coinciden con lo establecido anteriormente, pase a la siguiente sección.

En caso contrario, detenga el ensayo y compruebe:

Problema	Compruebe que
Pocillo blanco > 0.050 DO450nm/620-630nm	la solución cromógeno/substrato no se ha contaminado durante el ensayo.
CAL 1 0 arbU/ml > 0.150 DO450nm/620-630nm después de leer el blanco Coeficiente de variación > 30%	1. el proceso de lavado y los parámetros del lavador estén validados según los estudios previos de calificación. 2. se ha usado la solución de lavado apropiada y que el lavador ha sido cebado con la misma antes del uso. 3. no se han cometido errores en el procedimiento durante el dispensado del estándar. 4. no ha existido contaminación del Cal 1 o de sus pocillos debido a muestras positivas

	derramadas, o al conjugado. 5. las micropipetas no se han contaminado con muestras positivas o con el conjugado. 6. las agujas del lavador no estén parcial o totalmente obstruidas.
CAL 2 5 arbU/ml DO450nm/620-630nm < DO450nm/620-630nm CAL1 + 0.100	1. el procedimiento ha sido realizado correctamente. 2. no ha habido errores durante su distribución (dispensar el calibrador equivocado). 3. el proceso de lavado y los parámetros del lavador estén validados según los estudios previos de calificación. 4. no ha ocurrido contaminación externa del calibrador.
CAL 6 100 IU/ml < 1.000 DO450nm/620-630nm	1. el procedimiento ha sido realizado correctamente. 2. no ha habido errores durante su distribución (dispensar el calibrador equivocado). 3. el proceso de lavado y los parámetros del lavador estén validados según los estudios previos de calificación. 4. no ha ocurrido contaminación externa del calibrador.

De presentarse alguno de los problemas anteriores, luego de comprobar, avisar al supervisor para tomar las medidas pertinentes.

** Notas

Si se ha usado suero de control, comprobar los siguientes datos:

Parámetro	Exigencia
Suero Control	valor medio de DO450nm/620-630nm CAL4 ± 20%

Si los resultados de la prueba no se corresponden con los requisitos indicados anteriormente, proceder del siguiente modo:

Problema	Compruebe que
Suero Control Diferente de establecidos	1. el procedimiento ha sido realizado correctamente. 2. no ha habido errores durante su distribución (dispensar una muestra equivocada). 3. el proceso de lavado y los parámetros del lavador estén validados según los estudios previos de calificación. 4. no ha ocurrido contaminación externa del suero.


En cualquier caso, si todos los demás parámetros (blanco, CAL1, CAL2, CAL6) se corresponden con los requisitos establecidos, la prueba puede considerarse válida.

P. RESULTADOS.

P.1 Método cuantitativo.

Si el ensayo resulta válido, usar para el método cuantitativo un sistema de ajuste de curva para diseñar la curva de calibración con los valores obtenidos en la lectura a DO450nm/620-630nm (se sugiere interpolar 4 parámetros) y calcular sobre la curva de calibración la concentración de anticuerpos IgG al HSV presentes en la muestra.

A continuación, un ejemplo de curva de calibración:
Curva de calibración.

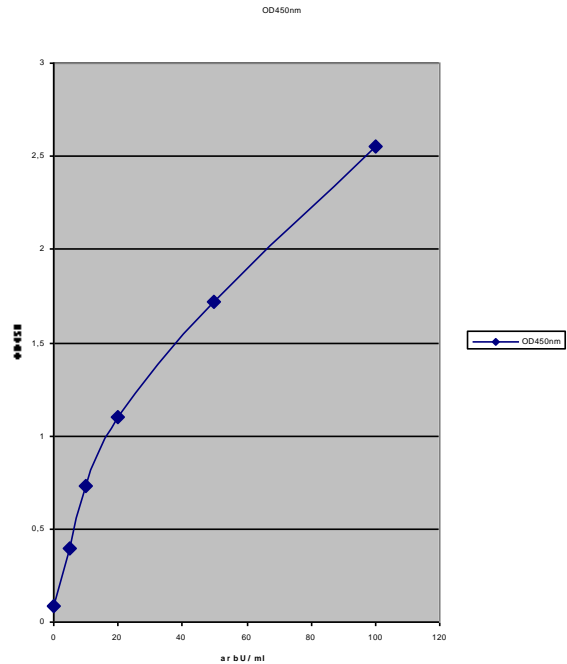

Nota Importante:

No usar la curva anterior para formular los cálculos.

P.2 Método cualitativo.

En el método cualitativo, calcular los valores medios de DO450nm/620-630nm para los Calibradores 0 y 5arbU/ml, luego comprobar que el ensayo es válido.

A continuación, un ejemplo de método cualitativo:

Los siguientes datos no deben usarse en lugar de los valores reales obtenidos en el laboratorio.

Calibrador 0 IU/ml: 0.020 – 0.024
Valor medio : 0.022 DO450nm/620-630nm
Menor de 0.150 – Válido

Calibrador 5 arbU/ml: 0.350 – 0.370
Valor medio: 0.36 DO450nm/620-630nm
Mayor que Cal 0 + 0.100 – Válido

Calibrador 100 arbU/ml: 2.245 DO450nm/620-630nm
Mayor de 1.000 – Válido

Q. INTERPRETACIÓN DE LOS RESULTADOS.

Las muestras con una concentración menor de 5 arbU/ml se consideran negativas a anticuerpos IgG anti-HSV.
Las muestras con una concentración mayor a 5 arbU/ml se consideran positivas a anticuerpos IgG anti-HSV.
Debe ponerse particular atención a la interpretación de los resultados ante sospecha de infección primaria por HSV en el embarazo, debido a las posibilidades de malformaciones del neonato.

Notas importantes:

1. La interpretación de los resultados debe hacerse bajo la vigilancia del supervisor del laboratorio para reducir el riesgo de errores de juicio y de interpretación.
2. Cuando se transmiten los resultados de la prueba, del laboratorio a otras instalaciones, debe ponerse mucha atención para evitar el traslado de datos erróneos.
3. En el monitoreo de infección por HSV durante el embarazo, un resultado positivo (presencia de anticuerpos IgG > 5 arbU/ml) debe ser confirmado para eliminar cualquier falso positivo o falsa definición de protección.

R. PERFORMANCES.

1. Límite de detección.

El límite de detección del ensayo ha sido calculado por medio de un Gold Standard Interno, en ausencia de una preparación internacional de referencia.

El límite de detección ha sido calculado como valor medio de DO450nm/620-630nm del Calibrador 0 arbU/ml + 5 SD.

La siguiente tabla muestra los valores medios de DO450nm/620-630nm del estándar, diluido en plasma negativo y examinado en el ensayo en tres lotes:

Valores medios de DO450nm/620-630nm (n = 2)

IgG arb/ml	HSVG.PU Lote 0203/2	HSVG Lote 0403/M	HSVG.PU Lote 0603
0	0.043	0.085	0.091
5	0.381	0.397	0.427
10	0.694	0.729	0.786
20	1.076	1.099	1.097
50	1.550	1.719	1.692
100	2.396	2.549	2.478

El ensayo muestra un límite de detección mucho mejor de 5 arbU/ml.

Para determinar el límite de detección y suministrar valores adicionales de sensibilidad analítica, se analizaron diluciones de la preparación Accurun n° 150, suministrada por Boston Biomedical Inc., BBI, Estados Unidos.

Valores medios de DO450nm/620-630nm (n = 2)

Dilución	HSVG.PU Lote 0203/2	HSVG Lote 0403/M	HSVG.PU Lote 0603
1 X	1.694	1.719	1.708
2 X	1.085	1.117	1.100
4 X	0.730	0.751	0.744
8 X	0.446	0.464	0.453
16 X	0.301	0.314	0.306
32 X	0.150	0.165	0.158
0 arbU/ml	0.043	0.085	0.066
5 arbU/ml	0.381	0.397	0.395

2. Sensibilidad Diagnóstica:

La sensibilidad diagnóstica se ha estudiado en un ensayo clínico externo utilizando paneles de muestras, clasificadas como positivas mediante un estuche de referencia US FDA. Se probaron muestras positivas correspondientes a diferentes etapas de la infección por HSV. El valor obtenido del análisis de más de 300 muestras fue > 98%. Por otra parte, el panel PTH 201, suministrado por BBI, fue evaluado con el estuche contra un panel de referencia FDA.

BBI Panel PTH 201 (Performance)

Panel ID #	Dia.Pro DO450nm/620-630nm	est. M/C o	REF HSV1 M/Co	REF HSV2 M/Co
01	1.064	2.7	3.5	1.6
02	2.525	6.4	2.9	4.4
03	0.860	2.1	1.0	1.1
04	2.391	6.0	4.4	4.1
05	1.793	4.5	4.0	2.2
06	1.093	2.8	0.8	1.4
07	0.801	2.0	0.9	1.2
08	2.180	5.5	2.9	3.9
09	2.086	5.3	4.6	3.4
10	0.029	0.1	0.3	0.3
11	1.900	4.8	3.8	2.7
12	0.995	2.5	2.1	2.3
13	1.833	4.6	2.4	3.3
14	0.153	0.4	0.4	0.5
15	2.130	5.4	4.7	3.6
16	1.320	3.3	1.9	2.7
17	3.008	7.6	4.6	5.6
18	1.042	2.6	2.8	1.6
19	0.097	0.2	0.3	0.3
20	0.414	1.0	0.6	0.8
21	1.682	4.2	3.3	2.2
22	2.364	6.0	5.1	4.1
23	1.926	4.9	4.3	2.2
24	1.556	4.0	1.6	2.5
25	2.372	6.0	5.1	3.7

Nota: Valor de corte = 5 arbU/ml = 0.395

3. Especificidad Diagnóstica :

La especificidad diagnóstica ha sido determinada en el mismo centro, utilizando paneles de muestras negativas provenientes de individuos sanos, clasificadas como negativas mediante un estuche de referencia US FDA.

Se emplearon además plasma sometido a métodos de tratamiento estándar (citrato, EDTA y heparina) y suero humanos para determinar la especificidad. No se ha observado falsa reactividad debida a los métodos de tratamiento de muestras.

Las muestras congeladas han sido probadas para comprobar si la colección y el almacenamiento interfiere con el procedimiento del ensayo. No se ha observado interferencia a partir de muestras limpias y libres de agregados.

Se analizaron muestras de interferencia potencial derivadas de pacientes con diversas patologías (mayormente positivos a ANA, AMA y RF) y de mujeres embarazadas. No se observaron reacciones cruzadas.

Se obtuvo un valor de especificidad total > 98% al examinar más de 100 muestras.

3. Precisión:

Ha sido calculada a partir del Calibrador 5 arbU/ml, considerado el valor de corte del ensayo, examinado en 16 réplicas en tres corridas separadas, para 3 lotes.

Los resultados son los siguientes:

HSVG: lote 0603/2

Valores medios	1ª corrida	2ª corrida	3ª corrida	Valor promedio
DO450nm/620-630nm	0.450	0.438	0.449	0.446
Desviación estándar	0.020	0.021	0.026	0.022
CV %	4.4	4.8	5.7	5.0

HSV.G.PU: lote 0603

Valores medios	1 ^{ra} corrida	2 ^{da} corrida	3 ^{ra} corrida	Valor promedio
DO450nm/620-630nm	0.449	0.441	0.453	0.448
Desviación estándar	0.024	0.024	0.029	0.026
CV %	5.4	5.4	6.5	5.8

HSV.G: Lote 0403/M

Valores medios	1 ^{ra} corrida	2 ^{da} corrida	3 ^{ra} corrida	Valor promedio
DO450nm/620-630nm	0.405	0.406	0.405	0.405
Desviación estándar	0.027	0.031	0.030	0.029
CV %	6.6	7.6	7.4	7.2

La variabilidad mostrada en las tablas no dió como resultado una clasificación errónea de las muestras.

S. LIMITACIONES DEL PROCEDIMIENTO.

La contaminación bacteriana o la inactivación por calor de la muestra pueden afectar los valores de DO y por tanto alterar los niveles del analito.

Las muestras que luego de ser descongeladas presentan partículas de fibrina o partículas agregadas, generan algunos resultados falsos positivos.

El ensayo es útil solo para probar muestras independientes y no mezclas.

El diagnóstico de una enfermedad infecciosa no debe establecerse en base a un solo resultado, sino que deben tenerse en consideración la historia clínica del paciente, la sintomatología, así como otros datos diagnósticos.

BIBLIOGRAFÍA.

1. Engvall E. and Perlmann P.. J.Immunochemistry 8: 871-874, 1971
2. Engvall E. and Perlmann P.. J.Immunol.. 109: 129-135, 1971
3. Remington J.S. and Klein J.O.. (1996) In "Infectious diseases of fetus and newborn infant". Sanders, Philadelphia, London, Toronto.
4. Volk W.A. (1982) In "essential of Medical Microbiology". 2nd ed., pp 729, G.B. Lippincott Co. Philadelphia, New York, S.José, Toronto.
5. Leinikki P.O. et al.. J.Clin.Microbiol.. 8:418, 1978
6. Piroid E. et al.. Révue Méd.Vet.. 131:25, 1980.
7. Vaheri A. et al.. J.Med.Virol.. 5:171, 1980.
8. Vejtorp M. et al.. Acta Path.Microbiol.Scand.. 88:349, 1980.
9. Voller A. et al.. Brit.J.Exp.Pathol.. 56:338, 1975

Todos los productos de diagnóstico in vitro fabricados por la empresa son controlados por un sistema certificado de control de calidad aprobado conforme a la norma ISO 13485. Cada lote se somete a un control de calidad y se libera al mercado únicamente si se ajusta a las especificaciones técnicas y criterios de aceptación de la CE.

Fabricante:
Dia.Pro Diagnostic Bioprobes S.r.l.
Via G. Carducci n° 27 – Sesto San Giovanni
(Milán) – Italia



